

# HCV Microlisa

Microwell ELISA Test for the Detection of Antibodies to Hepatitis C virus in Human Serum/ Plasma

## 1. INTENDED USE

The 3rd generation HCV Microlisa is an *in vitro* qualitative enzyme linked immunosorbent assay for the detection of antibodies against HCV (anti-HCVs) in human serum or plasma. The kit is basically intended to screen blood donations to identify and eliminate the infected units of blood and for clinical diagnostic testing.

## 2. PRINCIPLE OF THE ASSAY

The 3rd generation HCV Microlisa is based on a highly sensitive technique, Enzyme Linked Immunosorbent Assay which detects antibodies against HCV in human serum and plasma. The HCV proteins are present in serum at levels well below the limits of detection. Thus, immunodiagnosis of HCV infection is based on detection of host generated antibodies (anti-HCVs) to viral proteins.

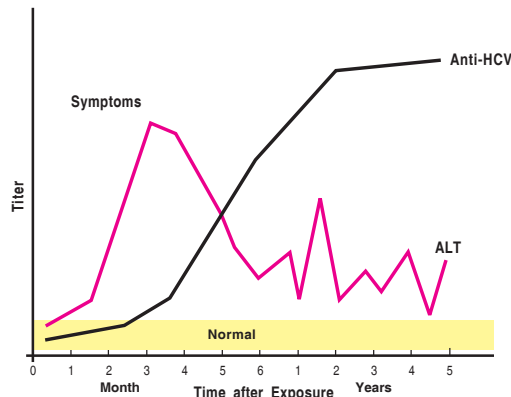


Fig. 1 Hepatitis C Virus Infection (Typical Serologic Course)

The 3rd generation HCV Microlisa utilises a combination of antigen with the sequence of both HCV structural and non-structural antigen i.e. CORE, E1, E2, NS3, NS4 and NS5. It has an obvious advantage over the available 2nd generation and 1st generation ELISA with improved sensitivity and specificity.

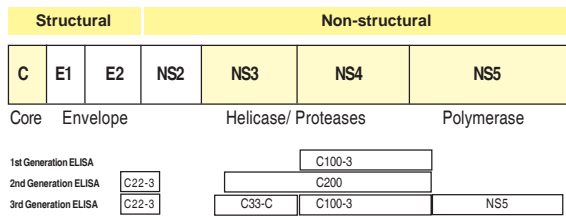



Fig. 2 Hepatitis C Virus Genome and Antigens used.

The combination of antigens for the structural and non-structural HCV proteins are coated onto the microwells (Fig.a).

Diluted sample and controls are then incubated. Antibodies to HCV, if present, bind to the immobilized HCV antigens on the microwell during this incubation period (Fig. b).

The microwells are then thoroughly washed with the diluted wash buffer to remove excess of unbound anti-HCV or other human IgGs which may interfere with the test. An enzyme conjugate, anti-human IgG conjugated with HRPO is added. The excess of enzyme conjugate is again removed with diluted wash buffer. At this stage the microwells hold only the bound antigen-anti HCV-enzyme conjugate complex (Fig. c).

In the next step, the freshly prepared substrate solution is incubated with the complex in the microwells. The enzyme substrate reaction leads to development of a blue colour which is indicative of the Ag-Ab reaction which has occurred in the microwell. In the final step the Stop Solution is added and the optical density of the developed colour is read photometrically (Fig.d).

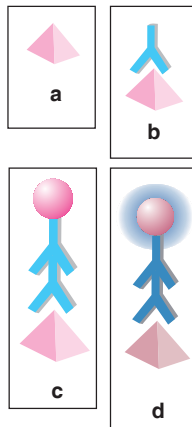

## 3. KIT PRESENTATION

96 Test Pack

## 4. KIT & ITS COMPONENTS

<b>Microwells</b>	12 Strips (12 X 8 wells) Breakway microwells coated with HCV antigens packed in a sealed pouch with dessicant.
<b>Sample Diluent</b>	1 Bottle (20 ml.) Buffer containing protein stabilizers and antimicrobial agents as preservative.

<b>Enzyme Conjugate Concentrate (100x)</b>	1 Vial (0.25 ml.) Anti-human IgGs conjugated with horseradish peroxidase with protein stabilizers.
<b>Conjugate Diluent</b>	1 Bottle (15 ml.) Buffer containing protein stabilizers.
<b>Wash Buffer Concentrate (25x)</b>	1Bottle (50 ml.) PBS with surfactant. Dilute 1:25 with distilled water before use.
<b>TMB Substrate</b>	1 Bottle (10 ml.) To be diluted with TMB diluent before use.
<b>TMB Diluent</b>	1 Bottle (10 ml.) Buffer solution containing H <sub>2</sub> O <sub>2</sub> with preservative
<b>Control -</b>	1 Vial (2.0 ml.) Ready to use, normal human serum negative for antibodies against HCV, HIV-1 & HIV-2 and HBsAg, containing sodium azide as preservative.
<b>Control +</b>	1 Vial (2.0 ml.) Ready to use, inactivated and diluted human serum; Reactive for HCV antibodies, non-reactive for HIV-1, HIV-2 and HBsAg containing sodium azide as preservative.
<b>Stop Solution</b>	1 Vial (15 ml.) Ready to use, 1N sulfuric acid.
<b>Plate Sealers</b>	Adhesive backed sheets for sealing microwell plate/strips.

## 5. STORAGE AND STABILITY

Store all components at 2-8°C when not in use. Expiry date on the kit indicates the date beyond which the kit should not be used.

## 6. ADDITIONAL MATERIAL AND INSTRUMENTS REQUIRED

- Micropipettes and microtips.
- Elisa reader
- Distilled or deionized water
- Graduated Cylinders, for reagent dilution
- Disinfectant solution
- Paper towels or absorbent tissue
- Timer
- Elisa washer
- Incubator 37°C
- Vortex Mixer
- Disposable gloves
- Glassware

## 7. SPECIMEN COLLECTION & PREPARATION

1. Only human serum or plasma samples should be used for the test. While preparing serum samples, remove the serum from the clot as soon as possible to avoid hemolysis. Fresh serum/plasma samples are preferred.
2. Specimens should be free of microbial contamination and may be stored at 2-8°C for one week, or frozen at -20°C or lower. Avoid repeated freezing and thawing.
3. Do not use heat inactivated samples as their use may give false results. Hemolyzed and icteric hyperlipemic samples may give erroneous results.

## 8. SPECIMEN PROCESSING

### (A) FROZEN SAMPLE

HCV Microlisa test is best used with fresh samples that have not been frozen and thawed. However most frozen samples will perform well if the procedure suggested below is followed.

Allow the frozen sample to thaw in a vertical position in the rack. Do not shake the sample. This allows particles to settle to the bottom. If a centrifuge is available, the sample should be centrifuged. (10,000 rpm for 15 min.)

### (B) TRANSPORTATION

If the specimen is to be transported, it should be packed in compliance with the current Government regulations regarding transport of aetiologic agents.

## 9. DESCRIPTION OF SYMBOLS USED

The following are graphical symbols used in or found on J. Mitra diagnostic products and packing. These symbols are the most common ones appearing on medical devices and their packing. They are explained in more detail in the European Standard EN ISO 15223-1:2016.

	Manufactured By		<i>In vitro</i> diagnostic medical device
	No. of tests		See Instruction for use
	Lot Number Batch Number		Temperature Limitation
	Manufacturing Date		Caution See instruction for use
	Expiry Date		Catalogue Number
	Do not use if package is damaged		Keep away from sunlight
	Keep Dry		

## 10. WARNING & PRECAUTION



**CAUTION:** THIS KIT CONTAINS MATERIALS OF HUMAN ORIGIN. NO TEST METHOD CAN OFFER COMPLETE ASSURANCE THAT HUMAN BLOOD PRODUCTS WILL NOT TRANSMIT INFECTION. NEGATIVE CONTROL, POSITIVE CONTROL & ALL THE SAMPLES TO BE TESTED SHOULD BE HANDLED AS THOUGH CAPABLE OF TRANSMITTING INFECTION.

1. The use of disposable gloves and proper biohazardous clothing is STRONGLY RECOMMENDED while running the test.
2. In case there is a cut or wound in hand, DO NOT PERFORM THE TEST.
3. Do not smoke, drink or eat in areas where specimens or kit reagents are being handled.
4. Tests are for *in vitro* diagnostic use only and should be run by competent person only.
5. Do not pipette by mouth.
6. All materials used in the assay and samples should be decontaminated in suitable disinfectant solution for 30-60 min. before disposal or by autoclaving at 121°C at 15psi for 60 min. Do not autoclave materials or solution containing sodium hypochlorite. They should be disposed off in accordance with established safety procedures.
7. Wash hands thoroughly with soap or any suitable detergent, after the use of the kit. Consult a physician immediately in case of accident or contact with eyes, in the event that contaminated material are ingested or come in contact with skin puncture or wounds.
8. Spills should be decontaminated promptly with Sodium Hypochlorite or any other suitable disinfectant.
9. Controls and Sample diluent contain Sodium Azide as a preservative. If these material are to be disposed off through a sink or other common plumbing systems, flush with generous amounts of water to prevent accumulation of potentially explosive compounds. In addition, consult the manual guideline "Safety Management No. CDC-22", Decontamination of Laboratory Sink Drains to remove Azide salts" (Center for Disease Control, Atlanta, Georgia, April 30, 1976.)
10. Stop solution contains sulfuric acid. If sulfuric acid comes in contact with the skin, wash thoroughly with water. In case of contact with eyes, flush with excess of water.
11. ELISA Reader & micropipettes used in testing should be calibrated at regular interval to ensure accurate results.

## 11. PRECAUTIONS FOR USE

**Optimal assay performance requires strict adherence to the assay procedure described in the manual.**

1. Do not use kit components beyond the expiration date which is printed on the kit.
2. Bring all the reagents & samples to room temperature (20-30°C) before use.
3. Do not combine reagents from different batches, as they are optimised for individual batch to give best results.
4. Avoid microbial contamination of reagents. The use of sterile disposable tips is recommended while removing aliquots from reagent bottles.
5. Due to interchange of caps the reagents may get contaminated. Care should be taken while handling the reagents to avoid contamination of any sort.
6. Use freshly collected, clean serum samples for assay. Try to avoid turbid, lipemic serum or plasma samples.
7. Use a separate tip for each sample and then discard it as biohazardous waste.
8. All pipetting steps should be performed with utmost care and accuracy. Cross contamination between reagents and samples will invalidate results.
9. Do not allow microwells to dry once the assay has started.
10. Run negative and positive controls in each assay to evaluate validity of the kit.
11. Incubation time should not vary by more than  $\pm 2$  min.
12. Prevent evaporation during sample incubation by covering the strips with strip sealer. Remove sealer before washing.
13. Distilled or deionised water must be used for wash buffer preparation.
14. Thorough washing of the wells is critical to the performance of the assay. Overflowing of reagents or washing to adjacent wells must be prevented during washing, which may lead to incorrect results due to carry over effect.
15. Take care while preparing working substrate solution as vials of TMB Substrate & Diluent are of same size.
16. Prepare working substrate solution just 10 minutes prior to adding in the wells.
17. If blue colour or white particles appear in working substrate solution then do not use it. Take fresh containers and tips and prepare it again.
18. Use separate tips for TMB Substrate and TMB diluent.
19. Avoid strong light exposure during the assay.
20. Ensure that the microwell strips are levelled in the strip holder. Before reading, wipe the bottom of the microwell strips carefully with soft, absorbent tissue to remove any moisture.
21. If available, a microwell reader which contains a reference filter with settings at 620 or 630 nm should be used. Use of a reference filter minimises interference due to microwells that are opaque, scratched or irregular. However, if a reference filter is unavailable, the absorbance may be read at 450 nm without a reference filter.
22. In case of any doubt the run should be repeated.

## 12. PREPARATION OF REAGENTS

Prepare the following reagents just before or during assay procedure. Reagents and samples should be at room temperature (20-30°C) before beginning the assay. All containers used for preparation of reagents must be cleaned thoroughly and rinsed with distilled or deionized water. Pre-warm the incubator to + 37°C.

### 12.1 HCV Microlisa strips:

Bring foil pack to room temperature (20-30°C) before opening to prevent condensation on the microwell strips.

- a. Break-off the required number of strips needed for the assay and place in the well holder. Take the strip holder with the required number of strips, taking into account that one negative and three positive controls should be included in the run while opening the fresh kit. However for one or two strips, one negative and two positive control and for more strips at least one negative and three positive control should be included in each subsequent runs.
- b. **Unused wells should be stored at 2-8°C, with dessicant in a aluminium pouch with clamp & rod. Microwells are stable for 30 days at 2-8°C from the date of opening of sealed pouch, when stored with desiccant along with clamp & rod.**

**Caution:** Handle microwell strip with care. Do not touch the bottom exterior surface of the wells.

### 12.2 Sample Preparation:

#### 1. MICROWELL DILUTION:

- a) Pipette 100µl of sample diluent in to the microwell.
- b) Add 10µl of serum sample to be tested.
- c) Ensure thorough mixing of the sample with the sample diluent.

**Note:** Cryoprecipitate may appear in sample diluent. Please ignore them as they do not interfere with the working of the kit and result interpretation

### 12.3 Preparation of Wash Buffer:

- a) Check the buffer concentrate for the presence of salt crystals. If crystals are present in the solution, resolubilize by warming at 37°C until all crystals dissolve.
- b) Prepare at least 50ml. (2 ml. concentrated buffer with 48 ml. distilled or deionised water) of buffer for each HCV Microlisa strip used. Mix well before use.

Alternatively, mix 20ml. of 25X wash buffer concentrate with 480 ml. of distilled or deionized water. **Wash buffer is stable for 2 months when stored at 2-8°C.**

### 12.4 Preparation of Working Conjugate:

Dilute conjugate concentrate 1:100 in conjugate diluent. **Do not store working conjugate.** Prepare a fresh dilution for each assay in a clean plastic/glass vessel. Determine the quantity of working conjugate solution to be prepared from table below. Mix solution thoroughly before use.

No. of Strips	1	2	3	4	5	6	7	8	9	10	11	12
No. of Wells	8	16	24	32	40	48	56	64	72	80	88	96
Enzyme Conjugate Concentrate (µl)	10	20	30	40	50	60	70	80	90	100	110	120
Conjugate Diluent in (ml)	1	2	3	4	5	6	7	8	9	10	11	12

**Note:** In case any precipitate is found in conjugate diluent, it should be allowed to settle and the supernatant can be used for the test. The precipitate does not interfere with the working of the kit.

### 12.5 Preparation of working substrate solution :

Mix TMB substrate and TMB Diluent in 1:1 ratio to prepare working substrate.

No. of Strips	1	2	3	4	5	6	7	8	9	10	11	12
No. of Wells	8	16	24	32	40	48	56	64	72	80	88	96
TMB Substrate (ml)	0.5	1.0	1.5	2.0	2.5	3.0	3.5	4.0	4.5	5.0	5.5	6.0
TMB Diluent (ml)	0.5	1.0	1.5	2.0	2.5	3.0	3.5	4.0	4.5	5.0	5.5	6.0

**Do not store working substrate.** Prepare a fresh dilution for each assay in a clean plastic/glass vessel. Determine the quantity of working substrate solution to be prepared from table. Mix solution thoroughly before use. Discard unused solution. A deep blue color present in the substrate solution indicates that the solution has been contaminated and must be discarded.

## 13. WASH PROCEDURE:

1. Incomplete washing will adversely affect the test outcome.
2. Aspirate the well contents completely into a waste container. Then fill the wells completely with wash buffer avoiding overflow of buffer from one well to another and allow to soak (approx. 30 seconds). Aspirate completely and repeat the wash and soak procedure 5 additional times for a total of 6 washes.
3. Automated washer if used should be well adjusted to fill each well completely without over filling.
4. Tap upside down on absorbant sheet till no droplets appear on the sheet, taking care not to dislodge the wells.

## 14. TEST PROCEDURE

**Note:** Once the assay has started, complete the procedure without interruption. All the reagents should be dispensed in the centre of the well and the tip of the pipette should not touch the wall of the microwell.

Fit the strip holder with the required number of HCV Microlisa strips. **The instructions of the procedure must be strictly followed.** Arrange the assay control wells in a horizontal or vertical configuration. Configuration is dependent upon ELISA reader software.

- Add 100µl Negative Control in well No. A-1. Negative control is ready to use & hence no dilution is required.
- Add 100µl Positive Control in B-1, C-1 & D-1 wells. Positive control is ready to use & hence no dilution is required.
- Add 100µl Sample Diluent in each well, starting from E-1 well followed by addition of 10µl sample. (Refer **MICROWELL DILUTION**)
- Apply cover seal and incubate at 37°C ± 2°C for 30 mins. ± 2 minutes.
- While the samples are incubating, prepare working wash solution and working conjugate as specified in "preparation of reagents".
- After the incubation is over, wash the wells 6 times with working wash solution according to the wash procedure given in the previous section.
- Add 100 µl of Working Conjugate Solution in each well.
- Apply cover seal & incubate at 37°C ± 2°C for 30 mins. ± 2 mins.
- While conjugate is incubating, prepare substrate solution in last 5 minutes of incubation as specified in "preparation of reagents". **Protect from light.**
- Aspirate and wash the wells after incubation as described in step no. 6.
- Add 100 µl working substrate solution in each well.
- Incubate at room temperature (20-30°C) in dark for 30 mins.
- Add 100 µl of stop solution.
- Read absorbance at 450 nm and 630 nm in ELISA READER.

## 15. SUMMARY OF PROCEDURE

Dilute Serum Sample		Sample 10 µl	Sample Diluent 100 µl
Add control (RTU)*		100 µl	
Cover the plate & incubate		30 mins. at 37°C	
Wash		6 Cycles	
Prepare working conjugate		No of Strips 1 2 3 4 5 6 7 8 9 10 11 12 Enz. conc. (µl) 10 20 30 40 50 60 70 80 90 100 110 120 Diluent (ml.) 1 2 3 4 5 6 7 8 9 10 11 12	
Add Conjugate		100 µl	
Cover the plate & incubate		30 mins. at 37°C	
Wash		6 Cycles	
Prepare Chromogenic Substrate		No of Strips 1 2 3 4 5 6 7 8 9 10 11 12 TMB Substrate (ml) 0.5 1.0 1.5 2.0 2.5 3.0 3.5 4.0 4.5 5.0 5.5 6.0 TMB Diluent (ml.) 0.5 1.0 1.5 2.0 2.5 3.0 3.5 4.0 4.5 5.0 5.5 6.0	
Add Substrate		100 µl	
Incubate in dark		30 mins. at Room Temp.	
Add Stop Solution		100 µl	
Read Results		450 nm./630 nm.	

\* RTU - Ready to use

## 16. CALCULATION OF RESULTS

### Abbreviations

- NC** - Absorbance of the negative control  
**PC** - Absorbance of the positive control  
**PC $\bar{x}$**  - Mean absorbance of Positive Control

### TEST VALIDITY:

#### Positive Control Acceptance Criteria:

PC or PC $\bar{x}$  must be > 0.5. If it is not so, the run is invalid and must be repeated.

	-	1.897	B1 Well
PC	-	1.855	C1 Well
	-	1.858	D1 Well
Total		<u>5.610</u>	
PC $\bar{x}$	=	5.610/3	= 1.870

### Negative Control Acceptance Criteria:

NC must be < 0.150. If it is not so, the run is invalid and must be repeated.

### CUT-OFF VALUE

The cut-off value is calculated as below:

$$\text{Cut off Value} = \text{PCx} \times 0.23$$

$$\text{e.g. PCx} = 1.87 \text{ then}$$

$$\text{Cut off Value} = 1.87 \times 0.23 = 0.430$$

## 17. INTERPRETATION OF RESULTS

- Test specimens with absorbance value less than the cut-off value are non-reactive for Anti-HCV.
- Test specimens with absorbance value greater than or equal to the cut-off value are reactive for Anti-HCV.
- Test specimens with absorbance value within 10% below the cutoff should be considered suspect for the presence of antibodies and should be retested in duplicate.
- Specimens with absorbance value equal to or greater than the cut-off value are considered initially reactive. Original specimen should be retested in duplicate.
- If both duplicate retest sample absorbance value is less than cutoff value, the specimen is considered nonreactive.
- If any one of the duplicate retest sample absorbance value is equal to or greater than the cutoff or both duplicate retest value are equal to or greater than the cutoff, the specimen is considered reactive by the criteria of HCV Microlisa. Further confirmation by other EIA assays or confirmation assays (PCR) including RIBA is recommended.
- Specimens which are not repeatedly reactive, may have shown colour due to:
  - Carry over of a highly reactive sample due to contamination of pipette tips.
  - Substrate contamination
  - Inadequate wash or aspiration during wash procedure.

## 18. LIMITATIONS OF THE ASSAY

- The 3rd generation HCV Microlisa detects anti-HCV in human serum or plasma and is **only a screening test**. All reactive samples should be confirmed by supplemental assays like RIBA. Therefore for a definitive diagnosis, the patient's clinical history, symptomatology as well as serological data should be considered. The results should be reported only after complying with above procedure.
- The assay is only valid for serum and plasma from individual bleeds and not for pools of serum or plasma or other body fluids.
- The 3rd generation HCV Microlisa detects IgG type of anti-HCV. Therefore, samples from acute HCV infection may produce a false negative result due to absence of the same as IgG type of anti-HCV are produced later during infection.
- A non-reactive result does not exclude the possibility of exposure to or infection with HCV.
- For the best results, the usage and storage instructions should be strictly followed. Any deviation from the procedure may lead to incorrect results.
- A repeatable false reactive results may occur due to non-specific binding of the sample or conjugate to the well.
- The presence of anti-HCV does not imply a Hepatitis C infection but may be indicative of recent and / or past infection by HCV.
- Patients with auto-immune liver diseases may show false reactive results.

## 19. PERFORMANCE CHARACTERISTICS

- Performance of **3rd Generation** HCV Microlisa with reference to sensitivity and specificity has been determined by W.H.O., Geneva. The samples included in the panels for evaluation were from Latin American, Asian, European and African origin. The panels also included various sero conversion panels from Boston Biomedica Inc. (BBI), world wide performance panel and anti-HCV low titre performance panel. The evaluation indicate the following sensitivity and specificity:

**Sensitivity 100% Specificity 97.4%**

Ref.: WHO evaluation report dated 13<sup>th</sup> June 2001.

- The performance of **3rd Generation** HCV Microlisa is also evaluated by reference Medical college/ Institute as mentioned below:

	Sensitivity	Specificity
CMC Vellore, Chennai, India:	<b>100%</b>	<b>98.6%</b>
Centre for liver disease, Hyderabad, India:	<b>100%</b>	<b>100%</b>

This information is provided for the Scientific Community Enquiring for an independent evaluation other than company's in house evaluation. It is not for commercial or promotional purpose.

- The performance of **3rd Generation** HCV Microlisa is also evaluated in house with fresh as well as frozen samples from low risk as well as high risk groups by using a panel containing 1148 nos. of known serum samples (including 550 tough sera). Rigorous tests were done with samples from random blood donors, patients with diseases related to HCV and patients with diseases unrelated to HCV. The results of all the sera with a defined HCV status were fully comparable with those of **3rd Generation** HCV Microlisa. The results of the in-house study done are as follows:

No. of Samples	Status	HCV Microlisa + ve	HCV Microlisa - ve
407	All RIBA +ve	407	-
741	EIA -ve	2	739

**Sensitivity : 100%** (407/407 RIBA Positive sera)

**Specificity : 99.73%** (739/741 EIA Negative sera)

**Precision:** Within run (Intra assay) & between run (Interassay) precision have been determined by testing 10 replicates of ten samples - two HCV negative and eight HCV Positive (1 strong positive and 7 weak positive). The C.V. (%) of all the ten samples were within 10%.

**20. LIMITED EXPRESSED WARRANTY DISCLAIMER**

The manufacturer limits the warranty to the test kit, as much as that the test kit will function as an *in vitro* diagnostic assay within the limitations and specifications as described in the product instruction-manual, when used strictly in accordance with the instructions contained therein. The manufacturer disclaims any warranty expressed or implied including such expressed or implied warranty with respect to merchantability, fitness for use or implied utility for any purpose. The manufacturer's liability is limited to either replacement of the product or refund of the purchase price of the product and in no case liable to for claim of any kind for an amount greater than the purchase price of the goods in respect of which damages are likely to be claimed. The manufacturer shall not be liable to the purchaser or third parties for any injury, damage or economic loss, howsoever caused by the product in the use or in the application there of.

**21. REFERENCES**

1. Caypers, H.T.M. et. al. (1971) J. of Hepatology,13, 5.15.
2. Sayers, M.H. & Gretch D.R. (1993). J. Transfusion 30,809-13.
3. Halfon, P. et. al. (1997) J. Medical Virology. 52:391-395
4. Sarin, S.K. & Hess. G. (1998). Transfusion associated Hepatitis. CBS Publishers, New Delhi.
5. S. Osborne, E. Cecconato, S. Griva, F. Garetto, R. Calogero, C. Rosa and F. Bonelli : Expression in E. coli and purification of a chimeric p22-NS3 recombinant antigen of Hepatitis C Virus (HCV). Federation of European Biochemical Societies, Volume 324, number 3, 253-257.

**22. TROUBLE SHOOTING CHART**

PROBLEM	POSSIBLE CAUSE	SOLUTION
1. No colour developed at the end of assay	a) Any one reagent has been added in wrong sequence. b) Inactivated conjugate, improper storage of any contamination. c) Microplate inactivated, due to improper storage d) Inactivated substrate, improper storage or preparation e) Omission of any step in test procedure f) Incorrect (low) incubator temperature, timing or pipetting g) Improper preparation of enzyme conjugate (dilution error) improper mixing of reagents.	Follow the procedure meticulously & repeat assay. Check storage of enzyme conjugate and it should be free Keep unused strips in aluminium poly pouch with the dessicant pouch inside and proerly closed with clamp & rod. Use freshly prepared substrate solution. Recheck procedure, repeat assay Follow the procedure meticulously & repeat assay. Check incubator temperature, procedure & repeat assay Check procedure & repeat assay
2. High O.D. value of Negative control	a) Plate not stopped after 30 minutes of adding stop solution b) Same microtip used for Positive and negative controls c) Nonspecific attachment/ binding of other reagent while addition of next step.	Follow the procedure meticulously & repeat assay. Change micropipette tips while addition of negative/ positive control If plates get scratches/ aberrations during washing, non specific proteins may bind
3. Too much colour in all wells of the plate (high background)	a) Contaminated substrate b) Contaminated washing solution (1X). Poor quality of water used for diluting wash buffer conc. c) Over incubation of substrate and delay in addition of stop solution. d) Insufficient washing. i) Washing not consistent ii) Filling volume not sufficient. iii) Insufficient no. of wash cycles. iv) Contaminated wash device	Check substrate (TMB Diluent) it should be colourless. If blue in colour then discard and use clean disposable container. Check the container and quality of water used for dilution. Use of distilled water is preferred. Follow the procedure meticulously. Check wash device, fill the well close to the top. After washing, blot the microwells on absorbent tissue. Follow wash protocol meticulously

PROBLEM	POSSIBLE CAUSE	SOLUTION
4. Poor reproducibility	e) Use of wash solution from other manufacturer.	Use only HCV Microlisa wash solution.
	f) Working substrate not protected from light	Incubate the plate in dark after addition of substrate.
	a) Washing problems.	Check all 8 ports/ manifold for uniform flow of wash buffer. If there are blockage, clen the ports.
5. False Positive	b) Uncalibrated pipettes or tips not well fitted, improper pipetting/ dispensing.	Use only calibrated pipettes with well fitted tips & pipette carefully without bubbling.
	c) Interference in optical pathway due to Air bubbles. and repeat the readings.	Clean or dry the bottom of microwells, check for bubbles
	Beside 3a, b, c, d, e & f incorrect interpretation and calculation of final results	Check the calculation part given in the insert and correctly interpret.
6. False Negative/ low O.D. of Positive control & positive sample	a) Inadequate addition of substrate/conjugate solution.	Follow the procedure meticulously & repeat assay.
	b) Kit expired, reagent of different kit used.	Check the expiry of the kit before use.
	c) White particles in working substrate solution.	Discard the substrate and prepare the working substrate again in fresh tube.
	d) Uncalibrated pipettes, improper pipetting.	Use only calibrated pipettes with well fitted tips & pipette carefully without bubbling.
	e) Deterioration of Enzyme conjugate	Check storage of Enzyme conjugate. It shall be stored at 2-8°C.
	f) Stop solution is added before 30 minutes. Reaction terminated before 30 minutes.	Follow the test procedure meticulously.
	g) O.D. taken at incorrect wavelength.	Read O.D. values at 450 nm and 630 nm.
	h) Incorrect (low) incubator temperature, timing or pipetting	Check incubator temperature, procedure & repeat assay

*in vitro* diagnostic Reagent, not for medicinal use



**J. Mitra & Co. Pvt. Ltd.**

A-180-181, Okhla Ind. Area, Ph.-1, New Delhi-110 020, INDIA  
 Ph.: +91-11-47130300, 47130500  
 e-mail: jmitra@jmitra.co.in Internet: www.jmitra.co.in